

FIGURE 1A

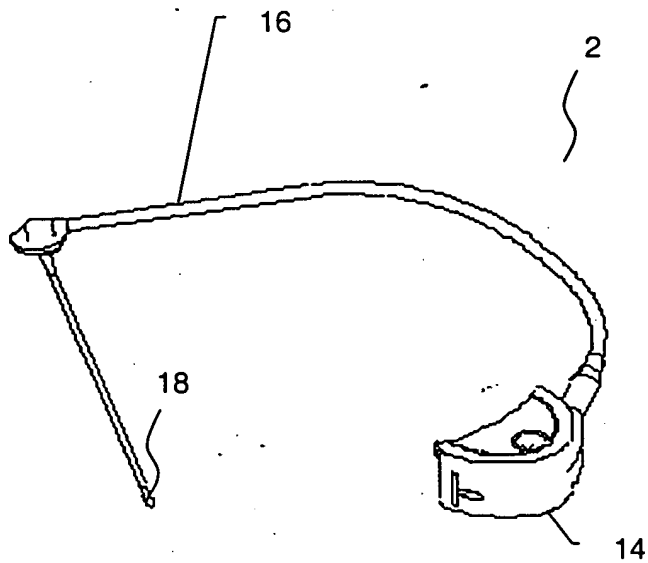


FIGURE 1B

09756196-080901

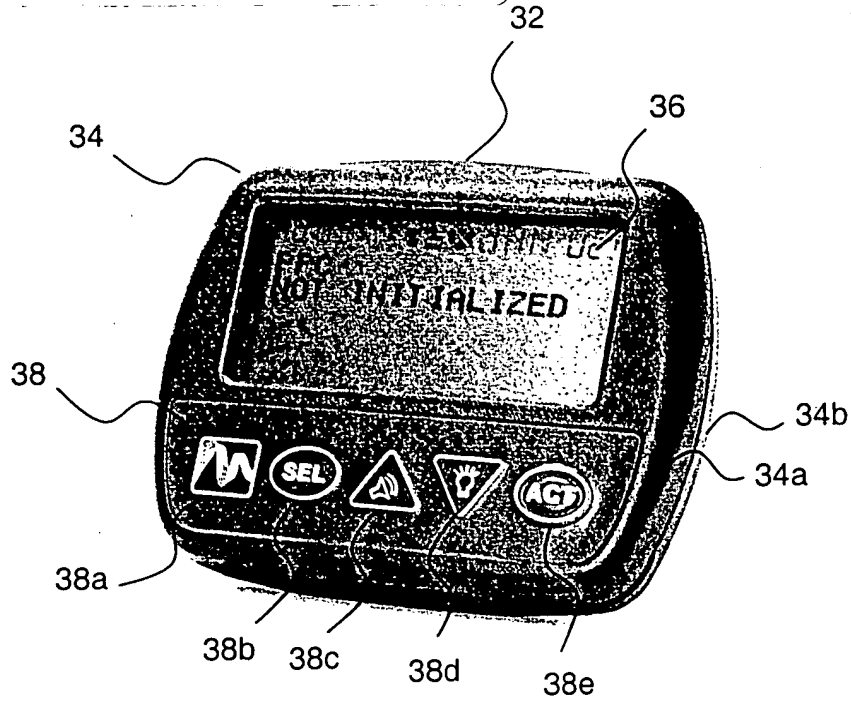


FIGURE 2

106080-96T89/60

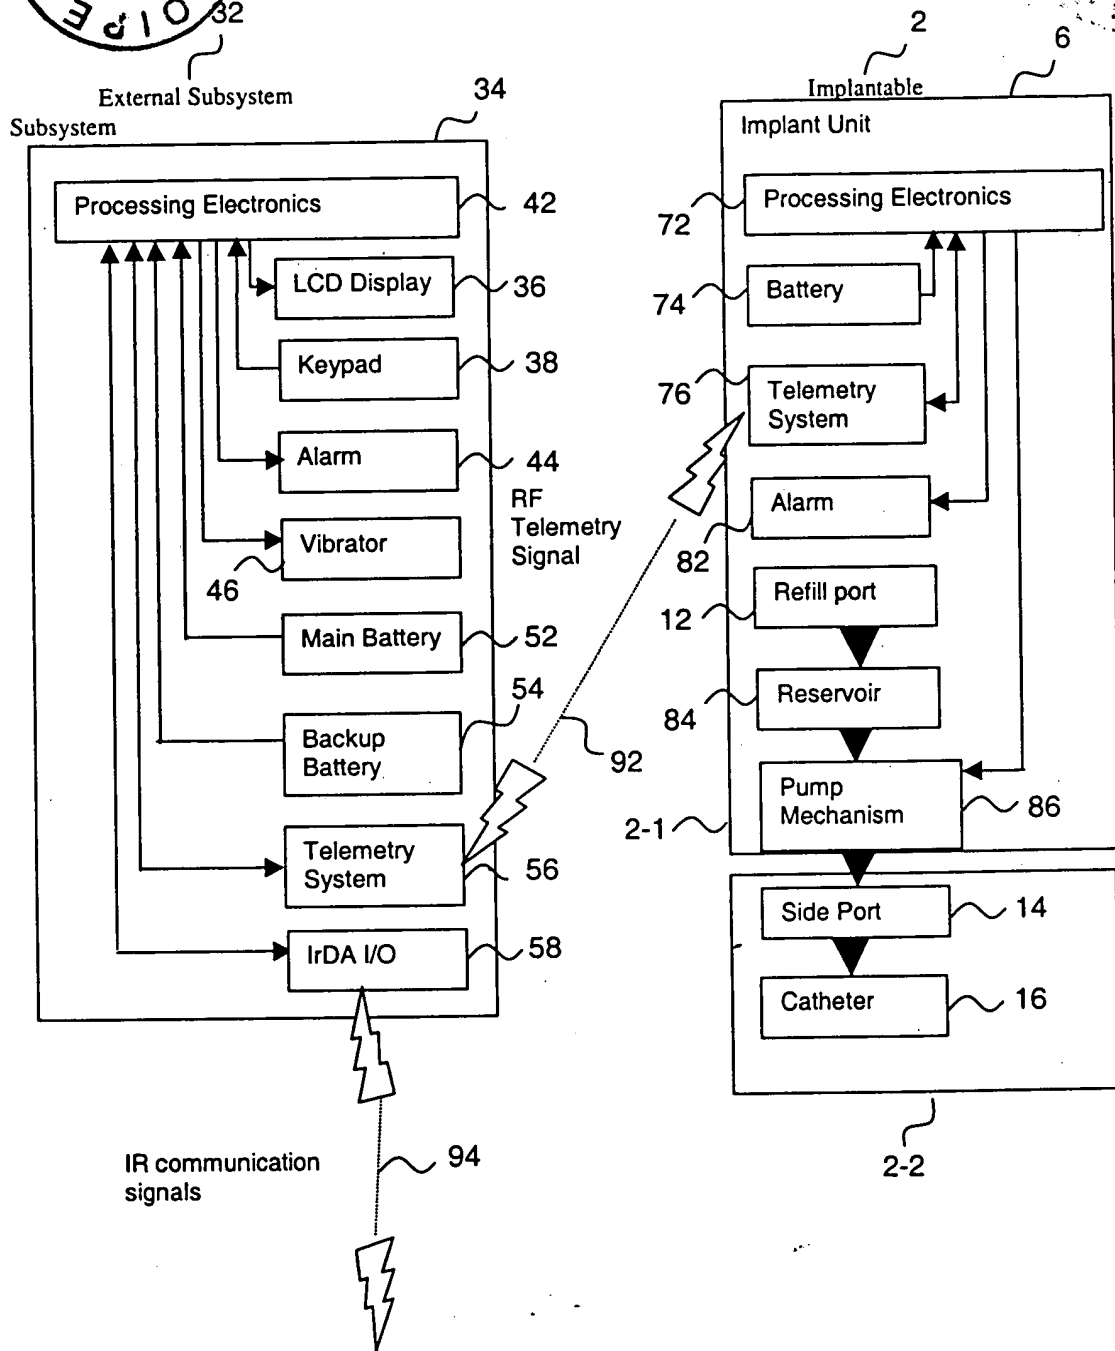



FIGURE 3

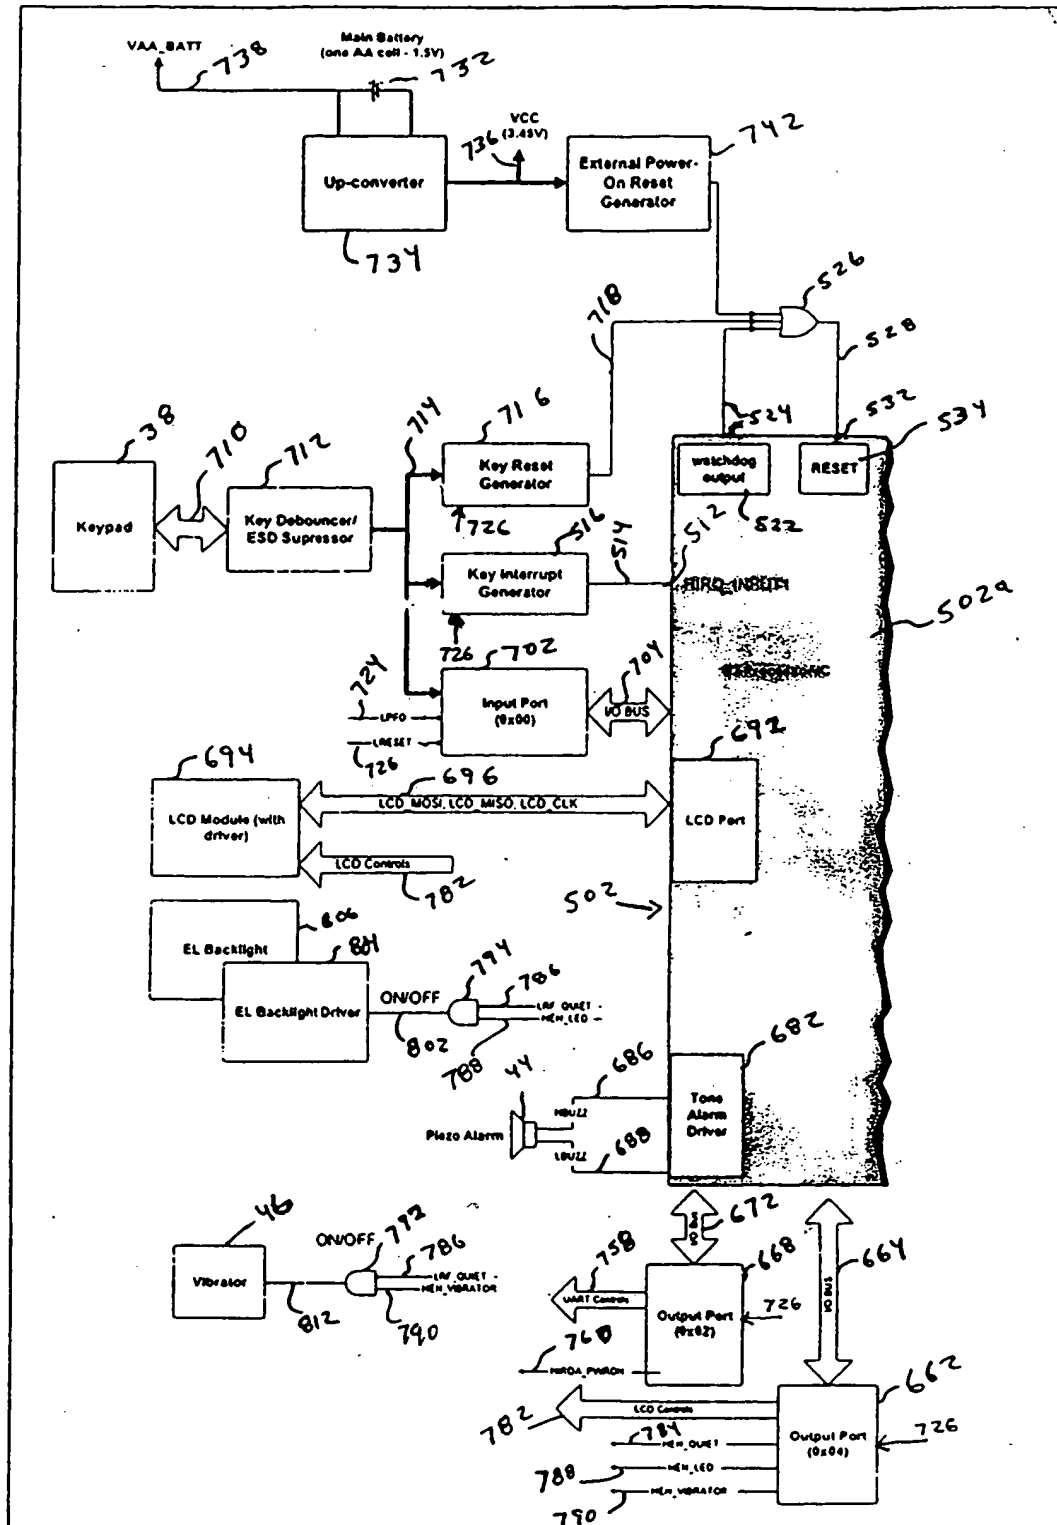


FIGURE 4a

09768196-0000

# AMBULATORY MEDICAL APPARATUS WITH HAND HELD COMMUNICATION DEVICE

Attorney: Ted Rittmaster - 047711-0221

Foley & Lardner - 310-277-2223

Sheet 5 of 16

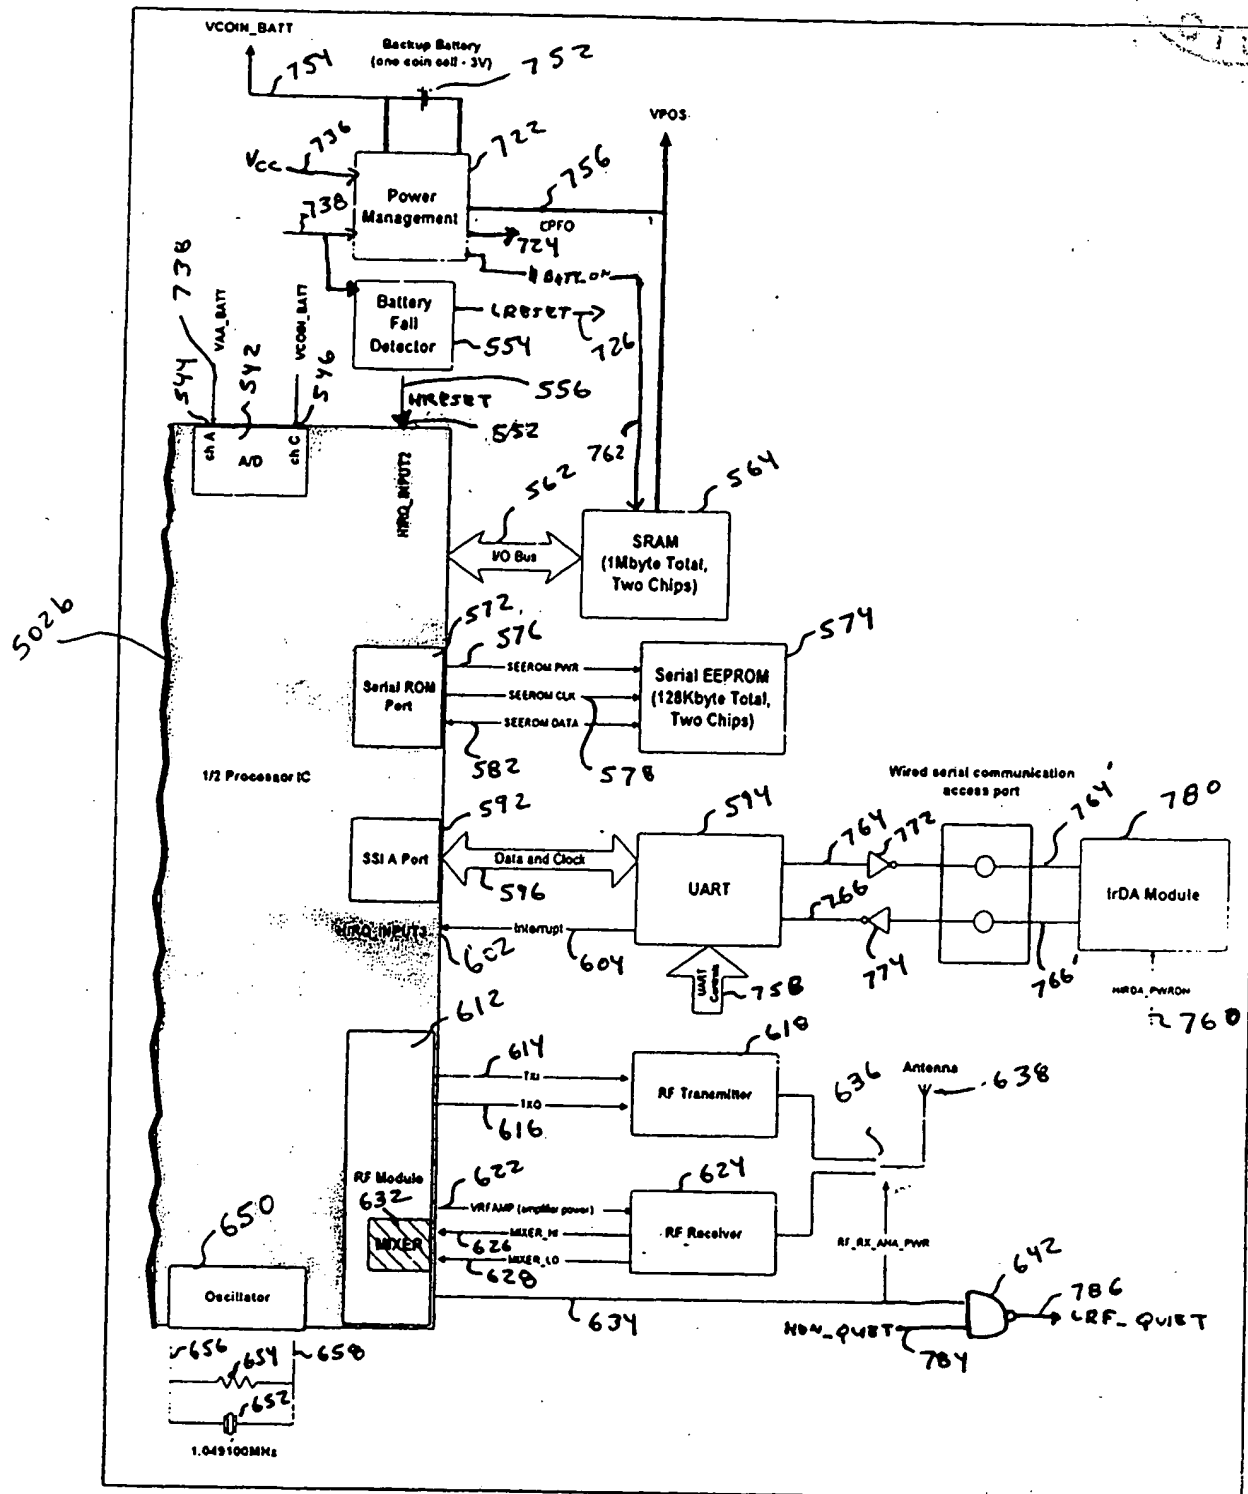






FIGURE 4b



- 88:88 ⇒ Time of Day
-  ⇒ Battery
-  ⇒ Alarm
-  ⇒ Reservoir Volume Level
-  ⇒ Delivery (Bolus/Basal)
- 888 ⇒ Month
- 88 ⇒ Date of Month

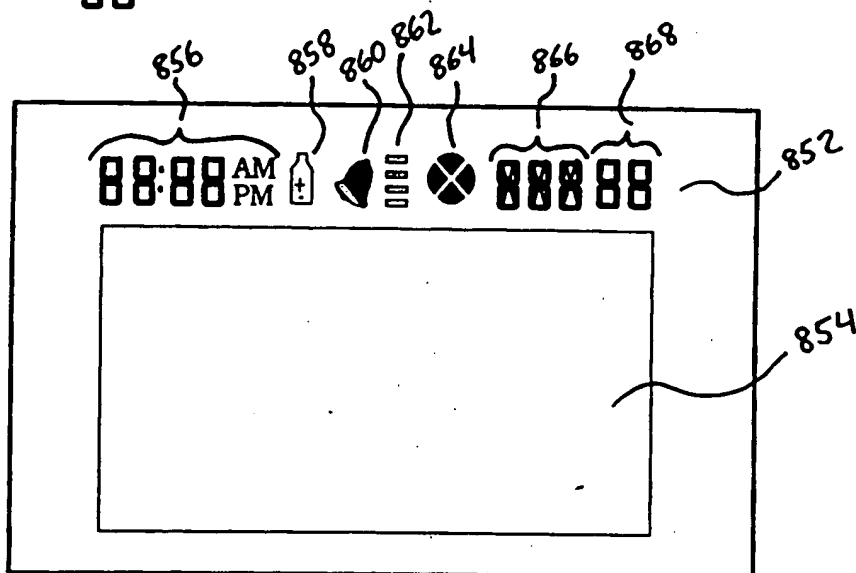


FIGURE 5

005080-96T89760

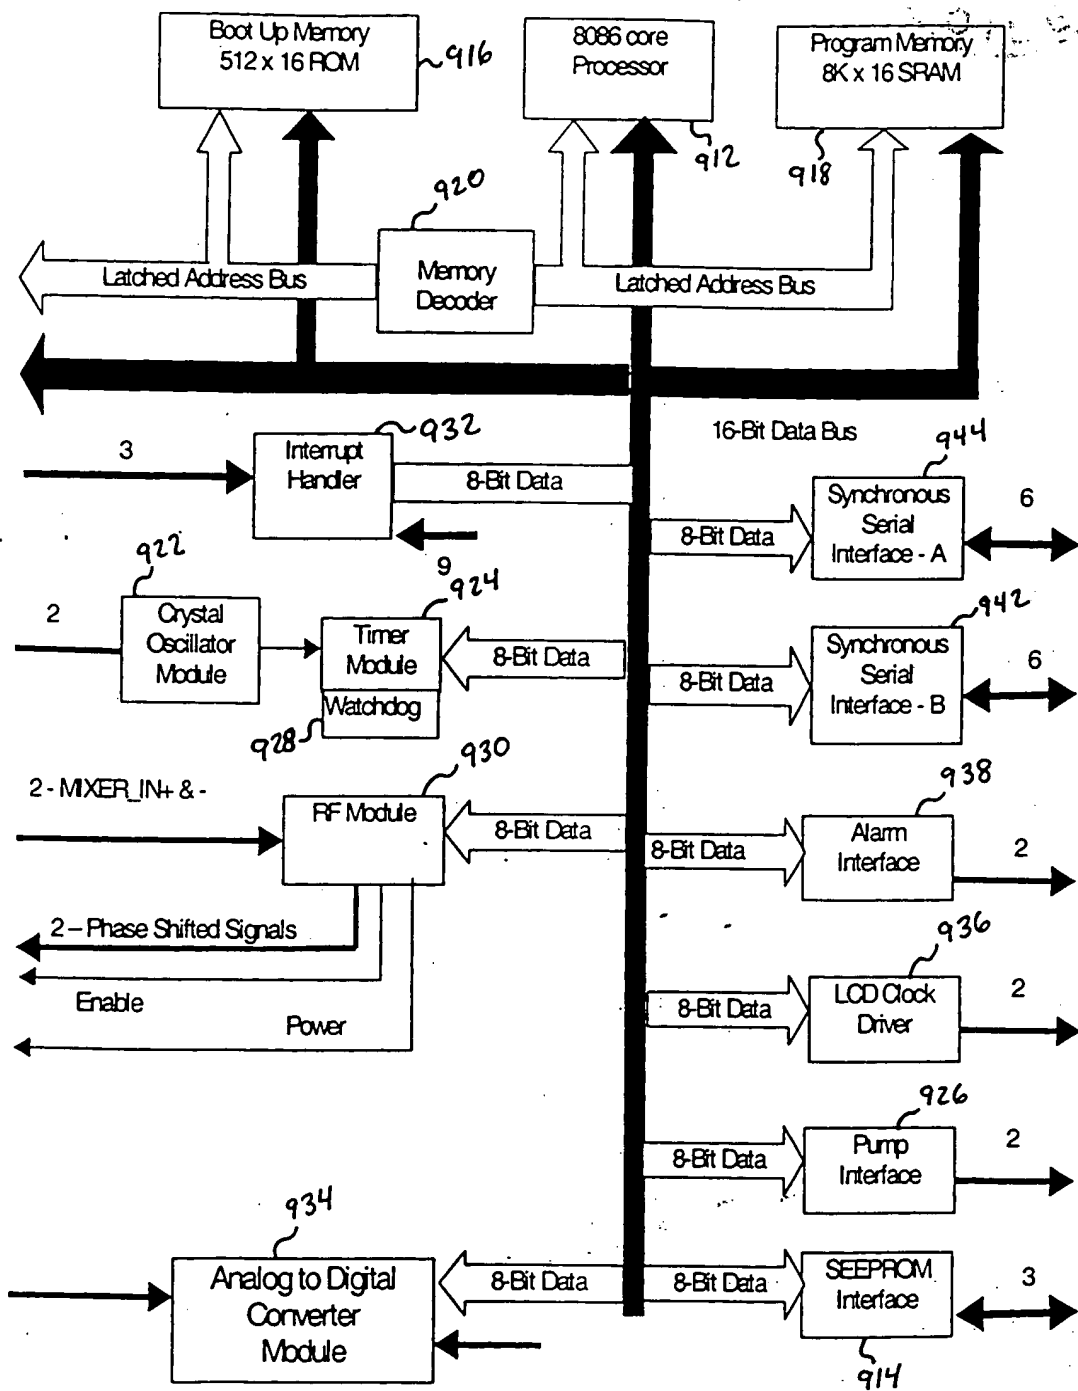


Figure 6

902

09768196-080901



## Main Menu

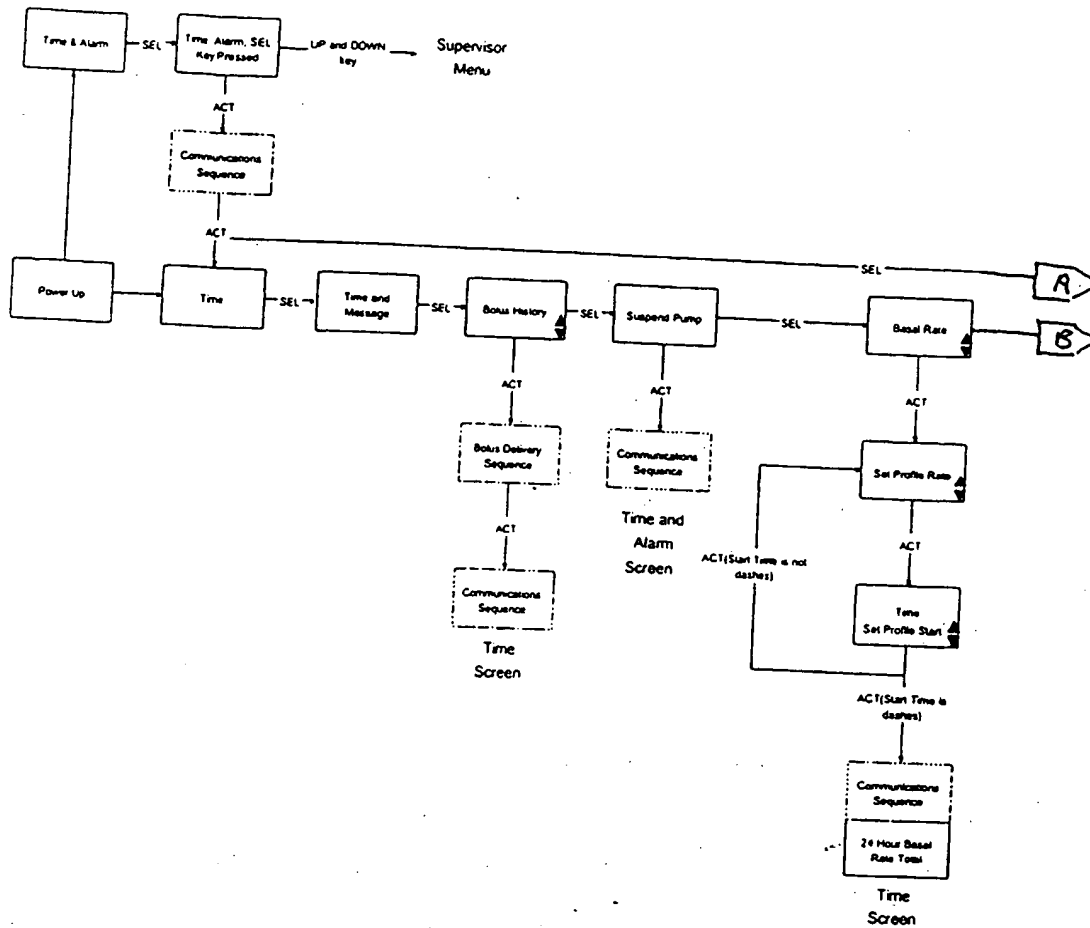


FIGURE 7a




AMBULATORY MEDICAL APPARATUS WITH  
HAND HELD COMMUNICATION DEVICE

Attorney: Ted Rittmaster - 047711-0221

Foley & Lardner - 310-277-2223

Sheet 9 of 16

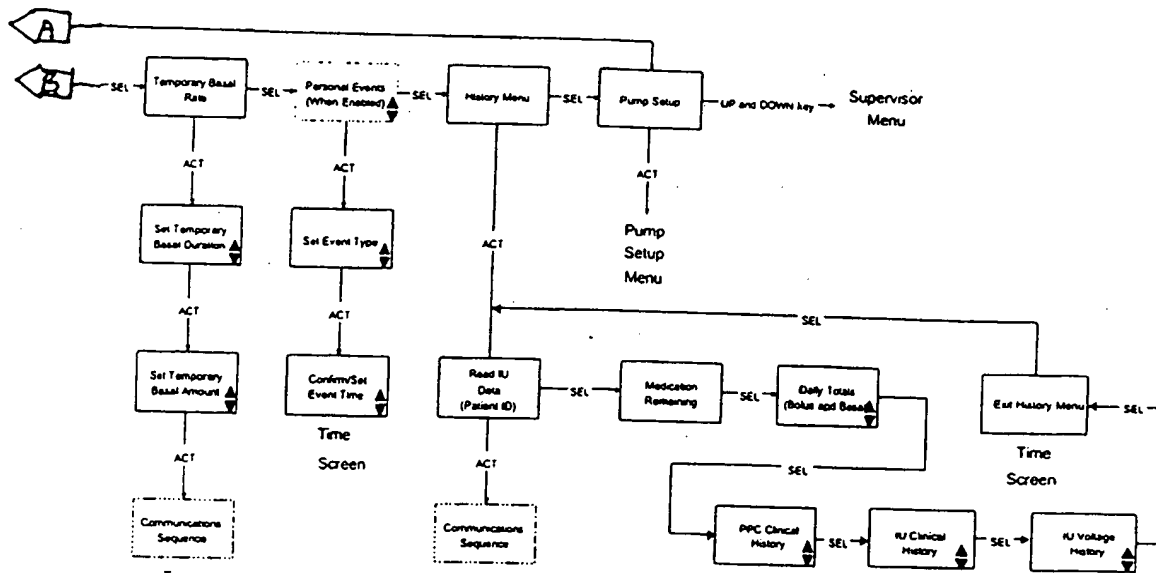

If the Communications Sequence on the History Menu is successful, the next screen in the menu shall be displayed.

FIGURE 7b



# Setup Menus

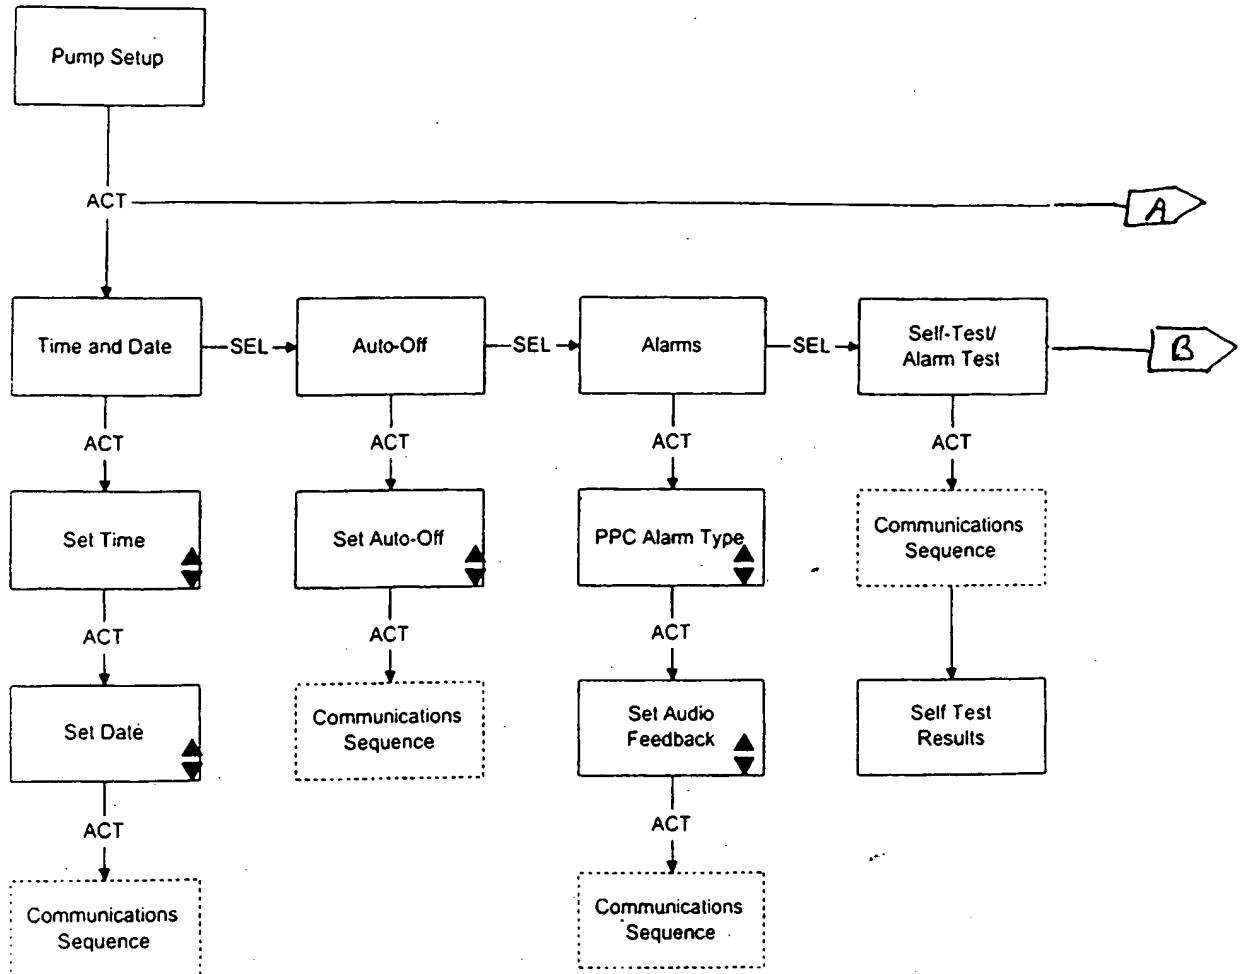


FIGURE 8a


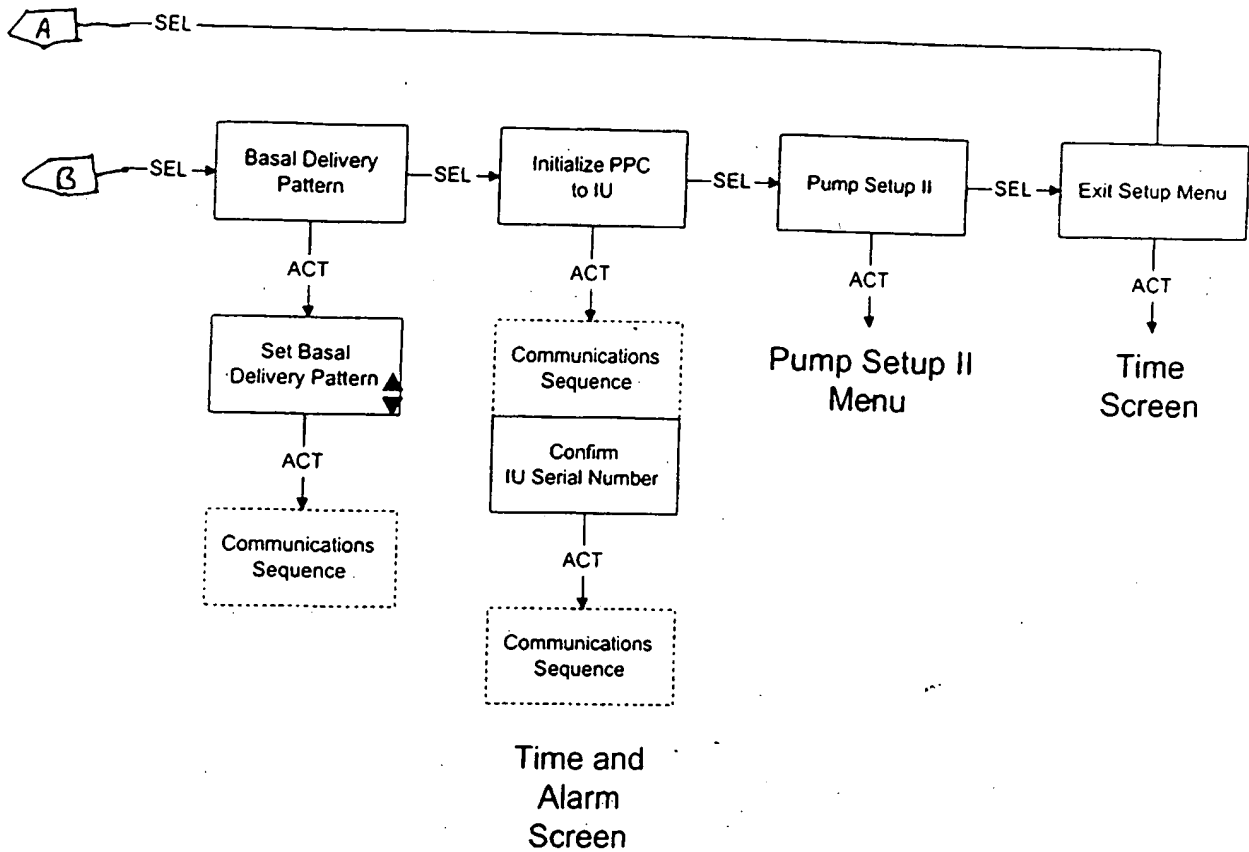


FIGURE 8b



# Pump Setup II Menu

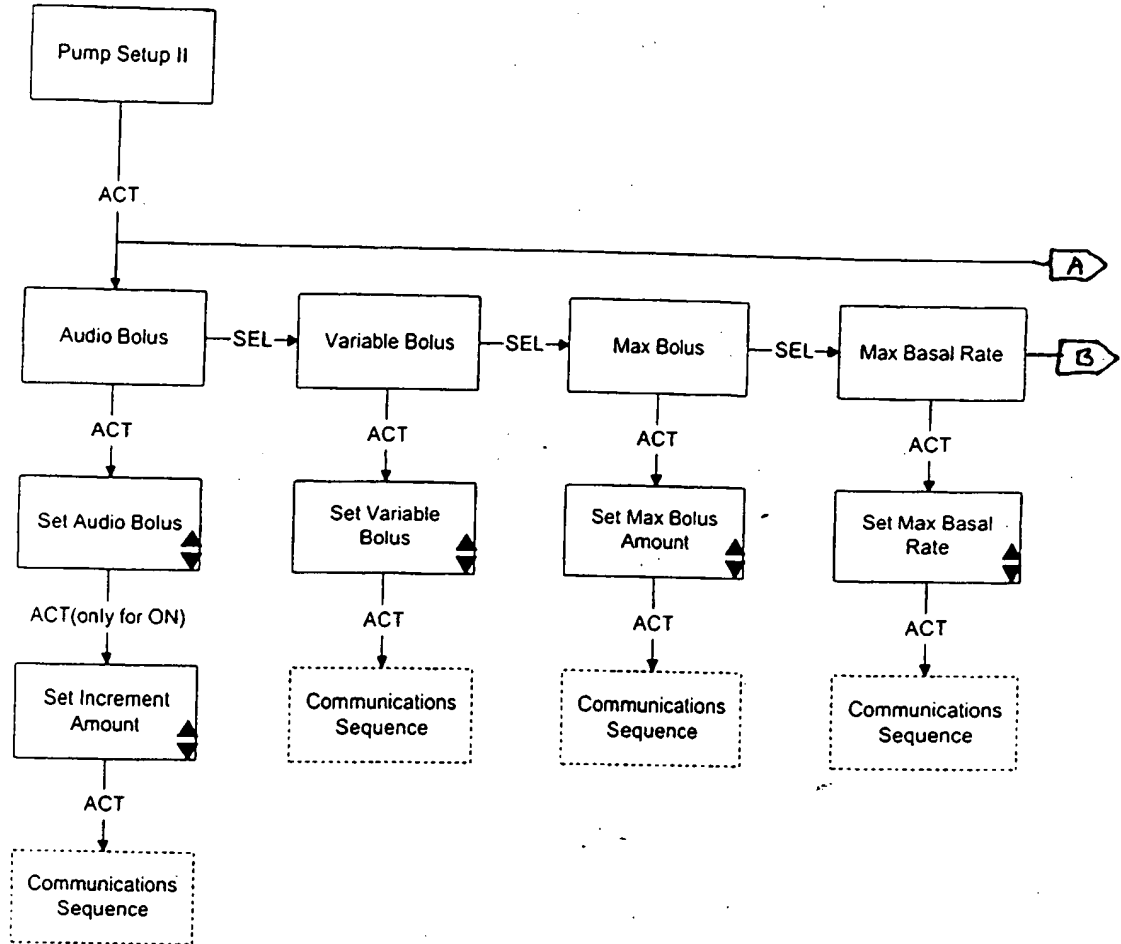

If the Communication Sequence is successful, the next screen in the menu shall be displayed.

FIGURE 9a


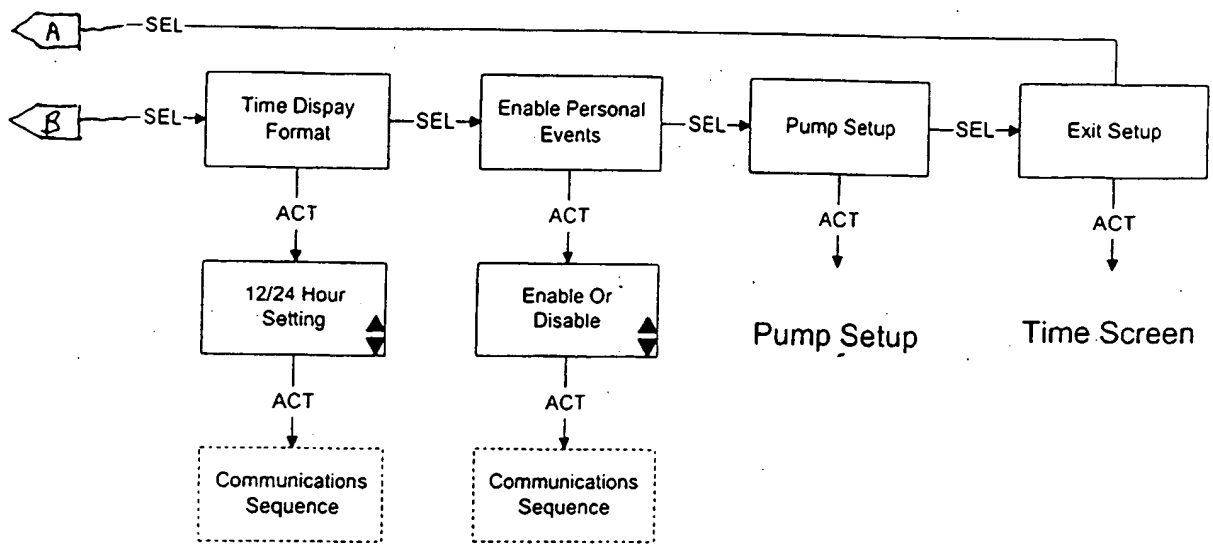


FIGURE 9b

09768195.080901



# Supervisor Menu

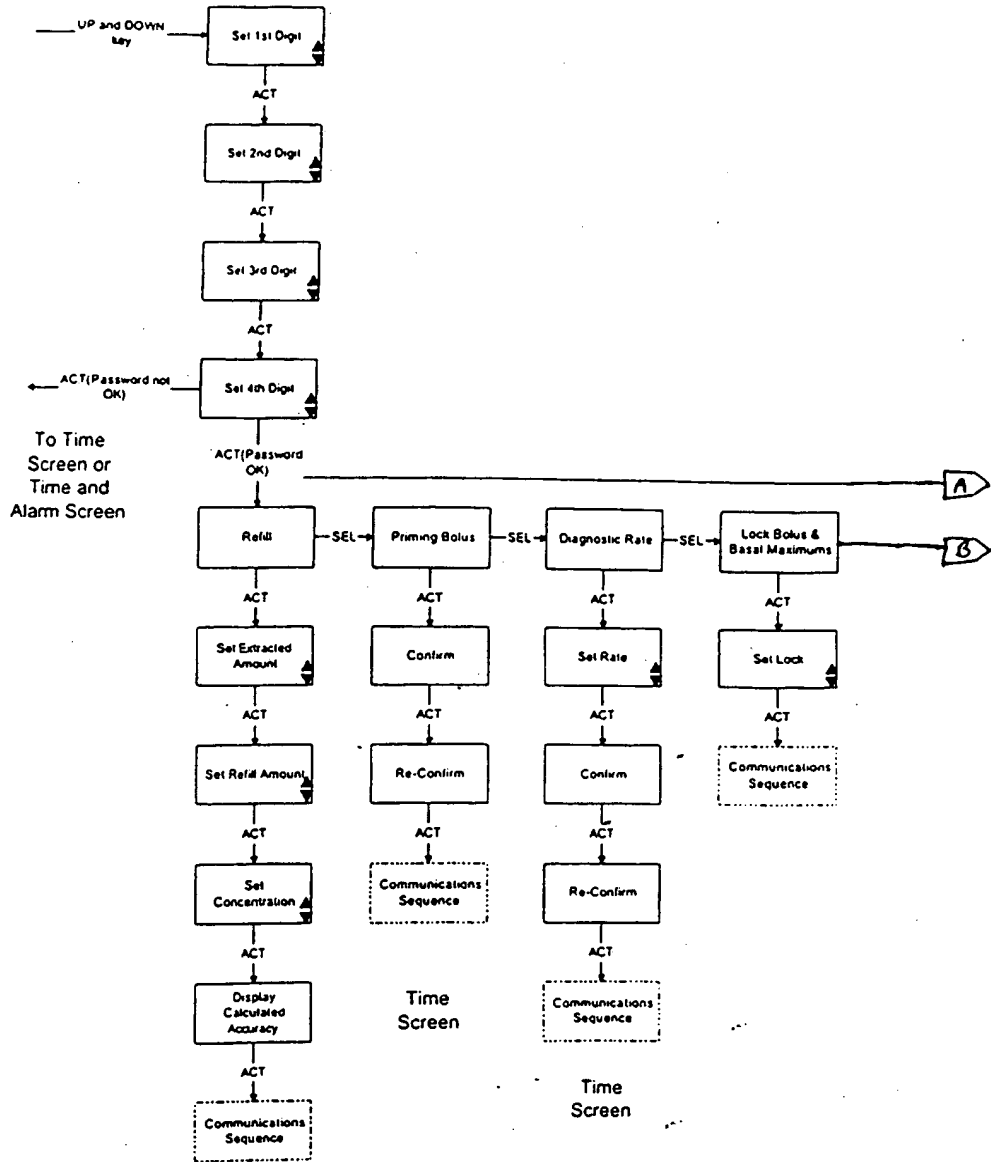

Unless otherwise shown, the screen that follows the Communications Sequence, shall be the next screen on the menu

FIGURE 10a

09769196 080901



09762195 000901

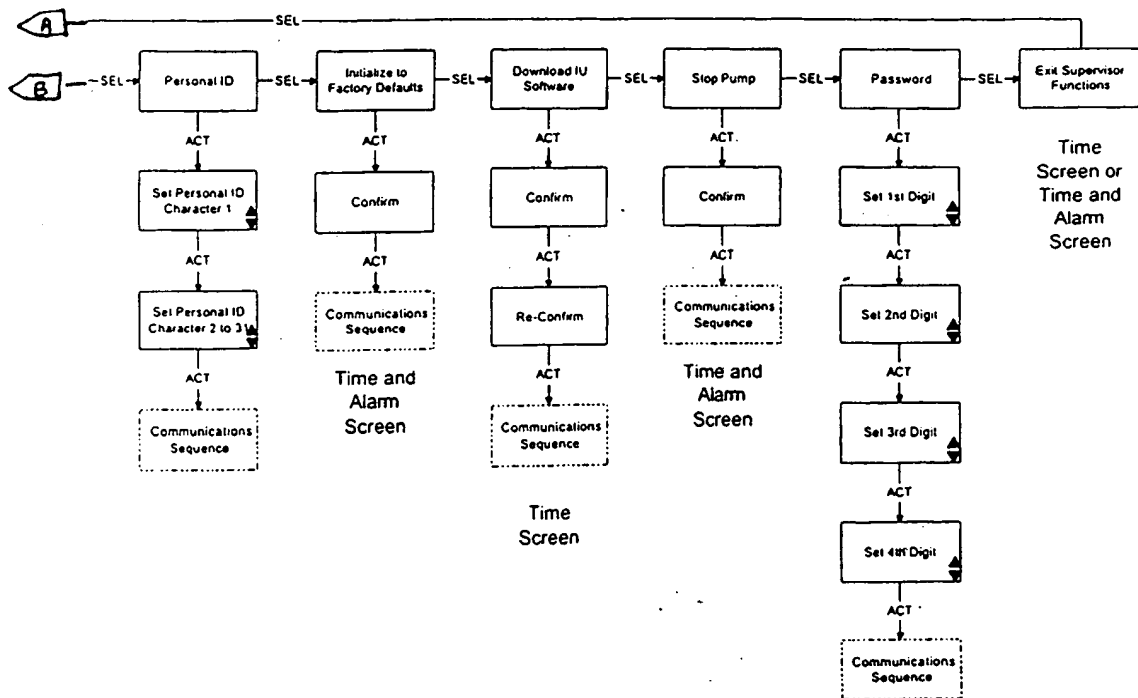


FIGURE 10b

TOP SECRET 91683260

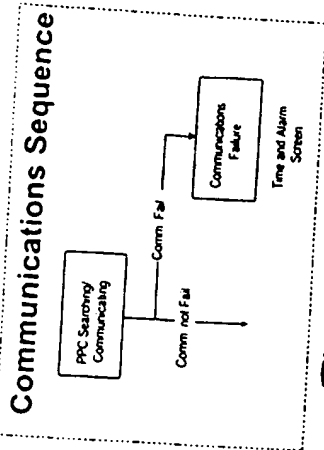



FIGURE 12

## Sequences

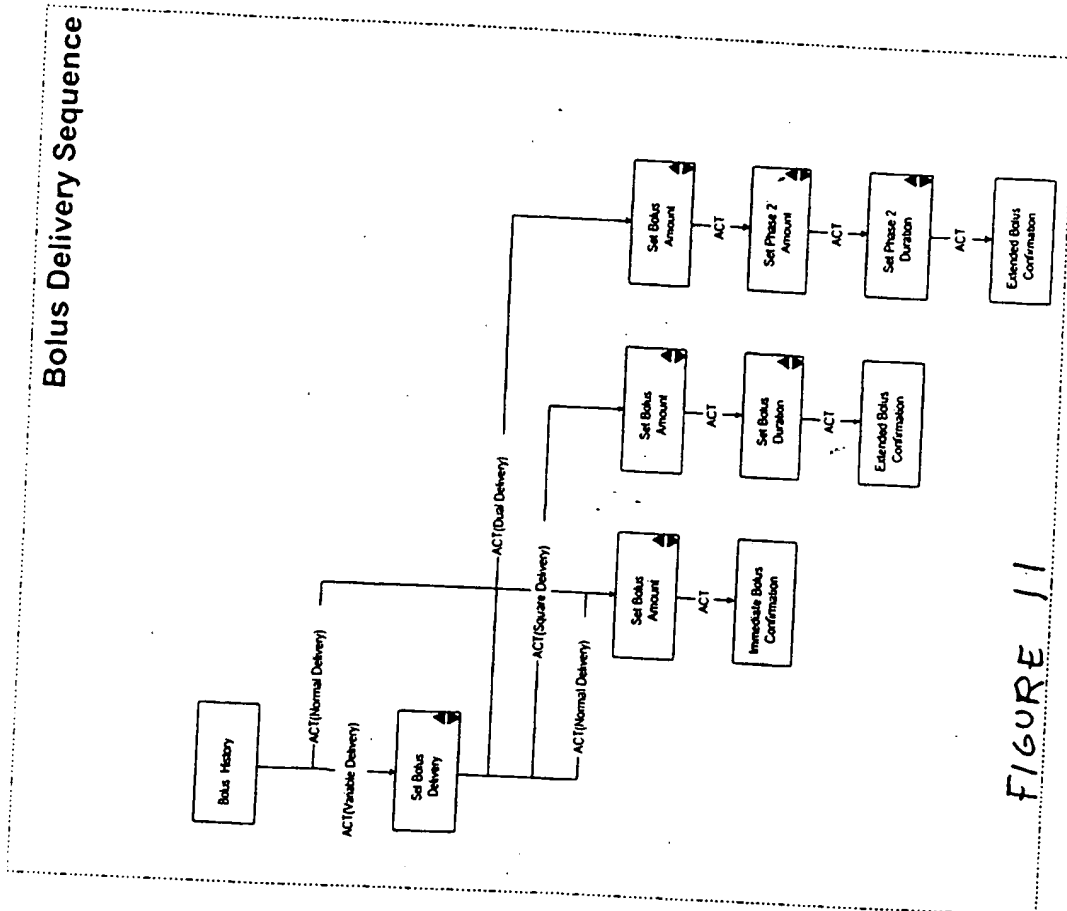


FIGURE 11